

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

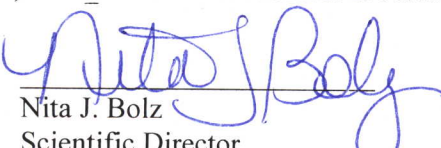
MAR 23 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130122 ✓
Name		TIM TUCKWOOD	ID# 3446 Date 3-16-10 ✓
A	Agency	Alaska State Troopers	Phone # 895-4800
Instrument Location		Delta Court	✓
Alco S/N		X301596 ✓	Target Value .081 ✓ High Pressure 400 psi ✓
B	Alco Test Value Average	083 ✓	082 ✓
		1 st Alco	2 nd Alco
Signature		Tim Tuckwood	
(OVER)			

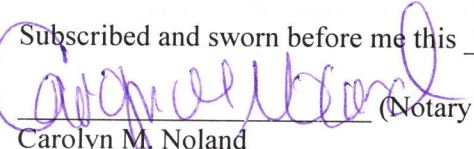
BMB
3/24/10

(Do Not write in the area below)


- I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
 - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
 - (3) I am the Scientific Director of the State Breath Alcohol Program.
 - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
 - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
 - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 15th day of April, 2010.


Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

(Notary Seal Stamp)



VERIFICATION OF CALIBRATION REPORT
of DataMaster cdm breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130122

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130122

MARCH 16, 2010

OPERATOR'S NAME:

TUCKWOOD TIM

OPERATOR'S NUMBER: 3446

SUBJECT'S LAST NAME:

VERIF

SUBJECT'S FIRST NAME/MI :

OF CAL

O.L. #: 12345

DEPT/AGENCY: DJTB

CASE/REPORT: 09876

TEST TYPE: U

ALCO TARGET VALUE: .001

— BREATH ANALYSIS —

.001 ADJUSTED FOR 29.21 in
ALCO TARGET .079 11:00
BLANK TEST .000 11:01
INTERNAL STANDARD VERIFIED 11:01
ALCO TU 29.21 in .003 11:02
BLANK TEST .000 11:02
SUBJECT SAMPLE .000 11:03
BLANK TEST .000 11:03
ALCO TU 29.21 in .002 11:04
BLANK TEST .000 11:04

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130122

MARCH 16, 2010
TIME 10:59

— DIAGNOSTIC CHECK —

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 40c

BREATH TUBE: 40c

BAROMETER: 29.21 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # \$ % ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~